

MATRIX **SURGICAL USA**

Where Art Meets Science



OMNIPORE[®] **SURGICAL IMPLANT**

Porous High-Density Polyethylene Implants
For Reconstructive and Aesthetic Surgery

OMNIPORE® Surgical Implant Handling Techniques

Implant Preparation

OMNIPORE Surgical Implants are sold sterile and should *never* be re-sterilized. Prior to handling the implants, operating room personnel should put on a clean pair of powder free gloves. Keep the implant in its protective packaging until time of implantation. Upon opening the inner pouch, the implant should be placed in a solution of clean sterile physiologic saline and antibiotics of the surgeon's preference. Strict adherence to the principles of aseptic technique should be followed with these implants. Proper surgical procedures and techniques are necessarily the responsibility of the medical professional.

Cutting

OMNIPORE Surgical Implants are easily cut with a variety of surgical instruments. The unique physical properties of the OMNIPORE Surgical Implants allows for cutting and trimming the implant while maintaining the interconnectivity and the structure of the pores. CAUTION: Do not place or carve the implant on surgical drapes, surgical clothing or any other surface which may contaminate the implant with lint and other particulate matter. A sterile carving block can be used as a work surface for carving OMNIPORE Surgical Implants.

Contouring & Shaping

Allow the implant to soak several minutes in a hot (above 90°C) saline bath. The hot saline bath will relax the memory of the implant, enabling modification of the shape. Test the implant for flexibility. Soak longer if the implant does not bend easily. Hold the implant in the desired shape and allow it to cool. A cold sterile saline bath can accelerate the cooling process. Repeat these steps if further modification is required.

Implant Stabilization

When fixation of the implant is desired, stabilization may be accomplished with suture, k-wire or rigid fixation screws. In the case of screw fixation, tightening the screw will compress the implant to the bone and will enable the surgeon to sink the screw head flush with the implant surface. One advantage of stabilizing the implant is the ability to delicately shape and feather the edges of the implant in-situ after fixation. Care should be taken to remove all carved debris from the surgical site.

Surgical Revisions

The porous nature of OMNIPORE Surgical Implants allows for soft tissue ingrowth and vascularization of the implant. In patients that may require later surgical revision, the surgeon should be aware of this vascular and soft tissue ingrowth. In the event revision or removal of the implant is required after ingrowth has occurred, the surrounding soft tissue may be raised with a surgical instrument and the implant dissected out with a scalpel or surgical scissors.

OMNIPORE Surgical Implants are provided sterile and should *never* be re-sterilized. Explanted OMNIPORE Surgical Implants should be disposed of in a proper biohazard container. Consult the product information sheet enclosed with each implant for additional information, indications, contraindications and precautions.

OMNIPORE® Surgical Implants

OMNIPORE implants are manufactured from a linear form of high-density polyethylene. Polyethylene has a long history of use in surgical implants. OMNIPORE Surgical Implants allow for tissue ingrowth because of its interconnecting open pore structure. The firm nature of the material allows carving with a sharp instrument without collapsing the pore structure. OMNIPORE Surgical Implants in blocks, sheets and preformed anatomical shapes are intended for augmentation and restoration of the craniomaxillofacial skeleton.

The porosity of OMNIPORE Surgical Implants is maintained large, with average pore sizes greater than 100 microns and pore volume in the 50% range (measured by Mercury Intrusion Porosimetry). Animal data has demonstrated that the OMNIPORE Surgical Implants permit tissue ingrowth. The clinical significance of tissue ingrowth may vary with the application and implant site. In Vitro and In Vivo biocompatibility studies have shown OMNIPORE Surgical Implants to be free from any observable systemic or cytotoxic effects.

The success of any implant is dependent upon careful handling and good surgical technique. Porous materials are particularly susceptible to contamination either by micro-organisms or foreign material. In order to reduce the chance of contamination by preoperative handling, OMNIPORE Surgical Implants are provided sterile in a variety of shapes and sizes. OMNIPORE Surgical Implants should remain in the protective pouch until the implant site has been prepared.

Select from an array of anatomical shapes, sheets/blocks and spheres including:


- Preformed shapes for chin, malar, rim, midface and mandibular augmentation
- Reconstructive shapes for traumatic defects and Microtic ears
- Sheets, wedges and blocks for orbital floor and wall repair
- Spheres for enucleation and evisceration procedures

A reference list of articles/presentations and publications on high-density polyethylene craniofacial implants and porous polyethylene is available upon request from Matrix Surgical USA.

Complete product labeling is included in the package insert provided with each OMNIPORE Surgical Implant. The surgeon should adequately review this information before using the product.

The intent of this brochure is to provide the surgeon with illustrations and dimensions of the many shapes of OMNIPORE Surgical Implants and ancillary surgical products. Implants can be tailored to accommodate the individual need of the patient.

Surgeons should utilize proper surgical techniques for which they were trained and their clinical experience to determine appropriate surgical procedures. Successful implantations are technique sensitive. Sound surgical judgment should be used in the selection/shaping and implantation of OMNIPORE Surgical Implants.

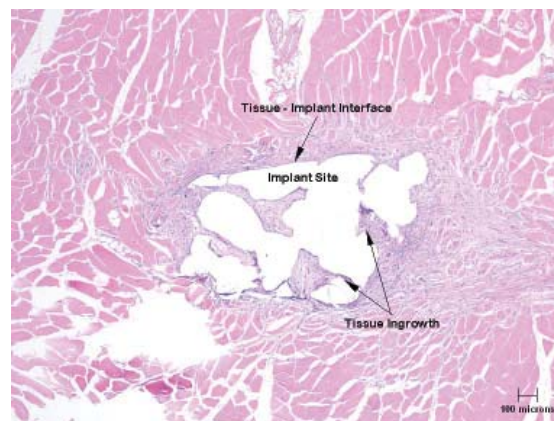

Design Y™ Facial Reconstruction and Cosmetic Implants


NEW

Design Y™ Mandible Onlays*

Designed in conjunction with Michael J. Yaremchuk, M.D.

Design Y Mandible Onlays benefit patients who have skeleton mandibular deficiencies or surgically altered anatomy. Implant design provides the opportunity for augmentation of ramus height and ramus width. It also provides the opportunity to alter the inclination of the mandibular plane and restore continuity of the mandibular border. The registration tab allows for ideal and symmetric placement. Three sizes with left and right orientation allow the surgeon to meet the requirements of each patient.

		A	B	C
OP7541	Design Y™ Mandible Onlay – Small – Left.....	57mm	x 39mm	x 5.0mm
OP7542	Design Y™ Mandible Onlay – Small – Right	57mm	x 39mm	x 5.0mm
OP7543	Design Y™ Mandible Onlay – Medium – Left	57mm	x 39mm	x 7.5mm
OP7544	Design Y™ Mandible Onlay – Medium – Right	57mm	x 39mm	x 7.5mm
OP7545	Design Y™ Mandible Onlay – Large – Left.....	57mm	x 39mm	x 10mm
OP7546	Design Y™ Mandible Onlay – Large – Right.....	57mm	x 39mm	x 10mm

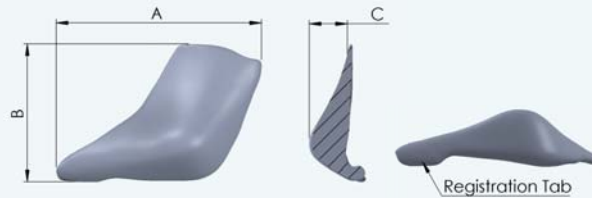

NEW


Design Y™ Chins*

Designed in conjunction with Michael J. Yaremchuk, M.D.

Design Y Chin implants come as a three-part assembly – right and left halves joined by a connecting tab – which allows for easier insertion. Two styles (round and square) are offered in a range of sizes to address patient needs. The Design Y Chin implants are uniquely designed with registration tabs which act as a flange to allow the implant to “hug” the inferior border of the mandible. Together with the connecting tab, the registration tabs allow for precise, symmetric augmentation of the chin complex. Implants can be easily trimmed and contoured to meet size requirements.

Design Y™ Chins

		A	B	C
OP8313	Design Y™ Chin – Small Round.....	35mm	x 32mm	x 4.0mm
OP8314	Design Y™ Chin – Medium Round	37mm	x 32mm	x 6.0mm
OP8315	Design Y™ Chin – Large Round	40mm	x 32mm	x 9.0mm
OP8316	Design Y™ Chin – Small Square	35mm	x 32mm	x 4.0mm
OP8317	Design Y™ Chin – Medium Square.....	37mm	x 32mm	x 6.0mm
OP8318	Design Y™ Chin – Large Square	40mm	x 32mm	x 9.0mm

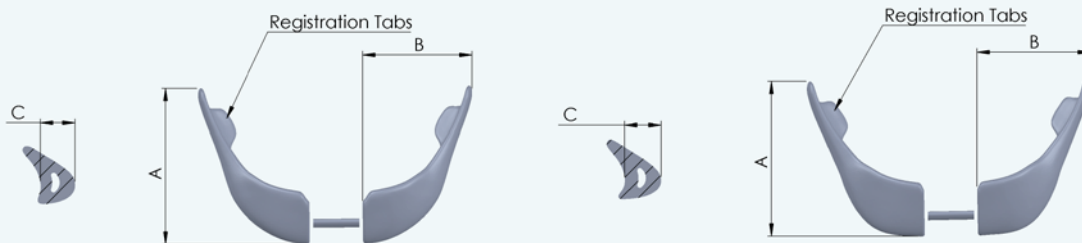

*U.S. Patent applications 13/532,283 and 12/342,762

Illustrations are not actual size; please consult dimensional descriptions.

Design Y™ Facial Reconstruction and Cosmetic Implants


NEW

Design Y™ Malars*

Designed in conjunction with Michael J. Yaremchuk, M.D.

Design Y Malars are used to reproduce normal contours of the facial skeleton. The Design Y Malar implants are uniquely designed with registration tabs which allow ideal and symmetric placement. Implants augment the projection of the malar prominence and extend from the infraorbital foramen, medially, to the zygomatico-temporal suture, laterally. They can be easily trimmed and contoured with a scalpel to meet specific patient requirements. Malars are available in a variety of sizes to minimize the need for alteration.


		A	B	C
OP9513	Design Y™ Malar – Small – Right	52mm	x 26mm	x 3.0mm
OP9514	Design Y™ Malar – Small – Left.....	52mm	x 26mm	x 3.0mm
OP9515	Design Y™ Malar – Medium – Right	52mm	x 27mm	x 4.0mm
OP9516	Design Y™ Malar – Medium – Left	52mm	x 27mm	x 4.0mm
OP9517	Design Y™ Malar – Large – Right	52mm	x 28mm	x 5.0mm
OP9518	Design Y™ Malar – Large – Left	52mm	x 28mm	x 5.0mm

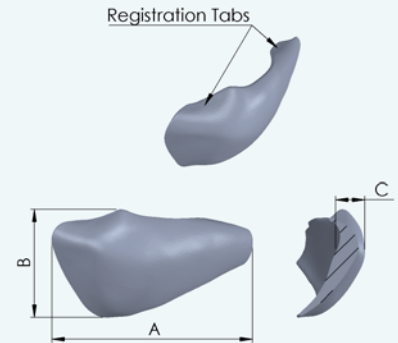

Design Y™ Inferior Orbital Rims

The Inferior Orbital Rim Implant can provide anterior projection and may be trimmed to the specific needs of the patient. A small flange assists with positioning of the implant on the most anterior aspect of the orbital floor. Screw fixation to the underlying skeleton is possible.


		A	B
OP9429	Inferior Orbital Rim – Left	48mm	x 25mm
OP9430	Inferior Orbital Rim – Right	48mm	x 25mm

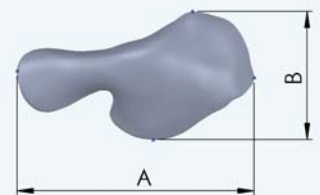

Extended Orbital Rims

The Extended Orbital Rim Implant can be used to augment the inferior and lateral orbital rim in trauma or for congenital cases. The implant allows for screw fixation for initial stabilization.

		A	B
OP9539	Extended Orbital Rim – Left	53mm	x 31mm
OP9540	Extended Orbital Rim – Right	53mm	x 31mm

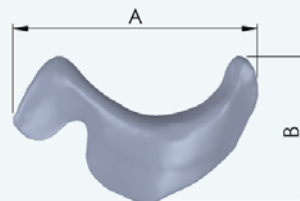

*U.S. Patent applications 13/532,283 and 12/342,762


Illustrations are not actual size; please consult dimensional descriptions.

Facial Reconstruction and Cosmetic Implants

Two-Piece Chin Designs

The Two-Piece Chin implant comes in two pieces: a right half and a left half. Segmentation facilitates easy placement of the implant. Designed for the reconstruction of the retrusive or hypoplastic chin, the two-piece design also provides flexibility and proper anatomical positioning of the implant. Implants are available in several anterior projections.


		A	B	C
OP8320	Two-Piece Chin – Small.....	62mm	x 27mm	x 5.0mm
OP8321	Two-Piece Chin – Medium	64mm	x 32mm	x 7.0mm
OP8322	Two-Piece Chin – Large.....	64mm	x 36mm	x 9.0mm

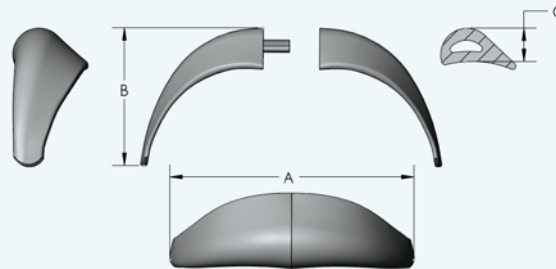

Osteotomy Gap Implant

The Osteotomy Gap Implant is designed to correct the inferior border contour irregularities of the mandible which inevitably occur after sagittal split osteotomy or sliding genioplasty. Each sterile package contains two implants.

		A	B
OP7550	Osteotomy Gap Implant.....	34mm	x 19mm

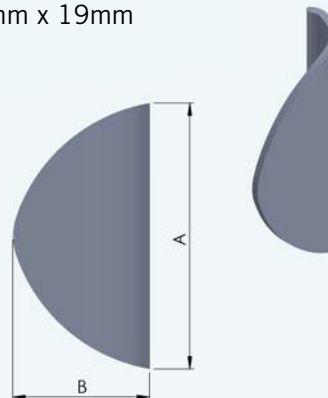

Microtia Reconstruction

Ear Implants


The OMNIPORE Base and Helical Rim Implants offer maximum flexibility to the surgeon in shaping the height and projection of the helix. The surgeon should always cover the entire implant with a vascular flap (i.e., temporal parietal fascia flap) followed by a skin graft to prevent late exposure of the implant. OMNIPORE Ear Implants are suitable for primary or secondary repair in both congenital and traumatic indications.

Ear Base Shapes

	A	B
OP8330 Ear Base Extended – Right	35mm	53mm
OP8331 Ear Base Extended – Left	35mm	53mm

Helical Rims

	A	B
OP8328 Helical Rim – Right	50mm	61mm
OP8329 Helical Rim – Left	50mm	61mm

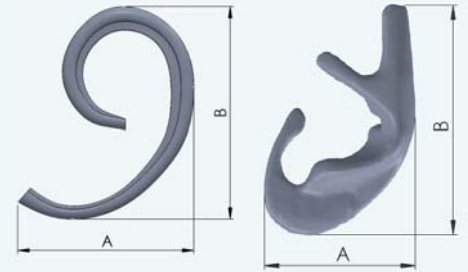


Nasal Reconstruction

Nasal Sheet

The Nasal Sheet is used to support tip elevation when nasal tip projection is needed. The Sheet is placed between the Medial Crura of the alar cartilage. Meticulous surgical technique should be used to prevent the implant from extending above the alar cartilage into the tip area.


	A	B	C
OP9536 Nasal Sheet	40mm	9mm	1.1mm

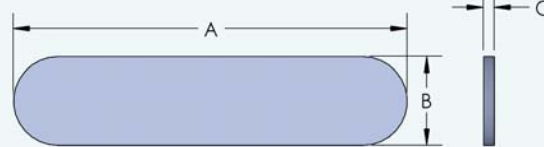

Paranasal Shapes

Crescent-shaped Paranasal Implants are designed to augment both the lateral and the inferior aspects of the piriform aperture. Implants can be carved to allow selective augmentation. The implants are available with right and left orientation and are available in two sizes.

	A	B	C
OP9519 Petite Paranasal – Left	29mm	19mm	6.0mm
OP9520 Petite Paranasal – Right	29mm	19mm	6.0mm
OP9525 Large Paranasal – Left	35mm	26mm	9.0mm
OP9526 Large Paranasal – Right	35mm	26mm	9.0mm




Temporal Hollowing

NEW

Pterional Implant

The Pterional Implant is used to correct temporal hollowing defects in patients who have had temporalis muscle atrophy due to surgical interventions through a pterional approach to the brain. The implant is placed deep to the temporalis when closing and can be secured with screw fixation to the surrounding temporal bone. Available in one size and left and right orientation, the Pterional Implant is smaller than the BENDBLOCK TF2 Implant, although similar in design.

		A	B	C	D
OP9864	Right	45mm	x 44mm	x 7.0mm	x 3.0mm
OP9865	Left	45mm	x 44mm	x 7.0mm	x 3.0mm

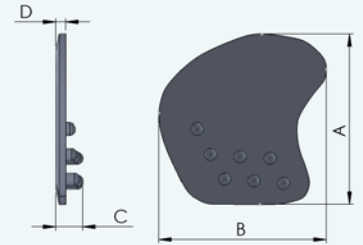


NEW

BENDBLOCK™ TF2 Implant

The BENDBLOCK TF2 Implant is designed to augment deficient soft tissue in the temporal region after trauma or when the temporalis muscle has been mobilized to a secondary site for reconstruction. Available in left and right orientation, the BENDBLOCK TF2 includes pedicles for volume enhancement that can be easily trimmed away with a scalpel depending on the specific needs of the patient.

		A	B	C
OP9857	TF2 Small – Left.....	76mm	x 61mm	x 19mm
OP9858	TF2 Small – Right.....	76mm	x 61mm	x 19mm
OP9859	TF2 Medium – Left	90mm	x 73mm	x 19mm
OP9860	TF2 Medium – Right	90mm	x 73mm	x 19mm
OP9861	TF2 Large – Left	101mm	x 85mm	x 19mm
OP9862	TF2 Large – Right	101mm	x 85mm	x 19mm

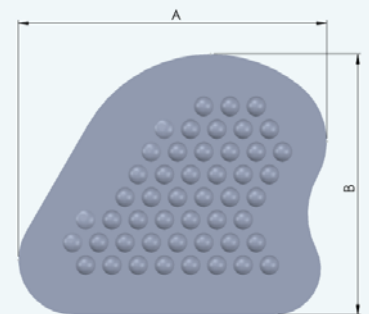


NEW

BENDBLOCK™ Implant

The BENDBLOCK Implant is designed for use in small or medium split-thickness cranial defects and contour deformities. The superior surface of the BENDBLOCK is smooth, while a pattern of pedicles on the inferior surface offer volume and flexibility. The implant can be modified with a scalpel to create a flange for fixation to the surrounding bone.

		A	B	C
OP6314	BENDBLOCK Implant	95mm	x 58mm	x 4.5mm

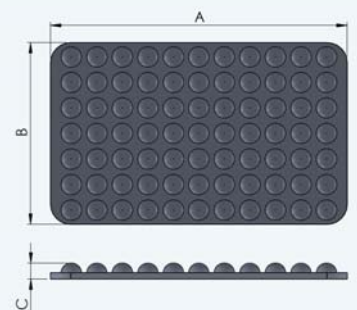

Illustrations are not actual size; please consult dimensional descriptions.

Cranial Reconstruction


NEW

Craniotomy Gap Wedge

Craniotomy Gap Wedge are implants designed to fit into the gap along a bone flap that is often left following a craniotomy. The top of the implant is shaped to extend over both sides of the gap and also allows for curvature. Each sterile package contains two implants.



	A	B	C	D
OP82011	Craniotomy Gap Wedge 102mm x 10mm x 4.7mm x 0.60mm			




NEW

Burr Hole Covers

Designed to fill and cover holes made by a cranial perforator, Burr Hole Covers are available in two sizes. The stems of the large cover allows for easy size modifications. The superior flange covers gaps between the cranial hole and the bone flap.



	A	B	C
OP7511	Burr Hole Cover <i>Coming soon</i>		
Quantity – 1			
OP7512	Burr Hole Cover 29mm x 15mm x 7.0mm		
Quantity – 1			

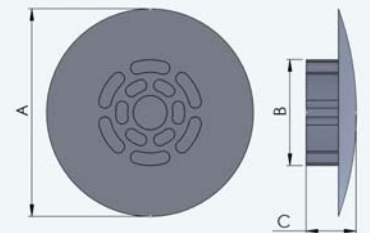


Sellar Buttress Implant (SBI™)

Used in repairing the floor of the sella turcica, the Sellar Buttress Implant (SBI) is available in two sizes and configurations. The small SBI comes with a single, protruding tab to facilitate handling and placement while the large SBI has three tabs to give the surgeon the flexibility to modify the implant without sacrificing any handling characteristics.



	A	B	C	D
OP82007	Sellar Buttress Implant 20mm x 20mm x 2.45mm x 0.45mm			
OP82008	Sellar Buttress Implant – Large 40mm x 40mm x 2.7mm x 0.70mm			

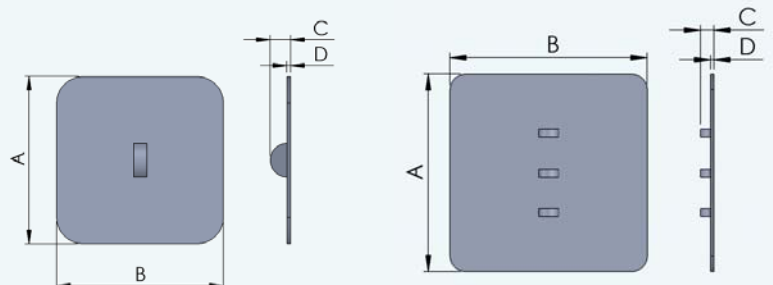

Cranial Reconstruction


NEW

BENDBLOCK™ Cranial Grid Implant

The BENDBLOCK Cranial Grid Implant is designed to fill full thickness cranial defects. The inferior surface's waffle-pattern design provides strength and flexibility, while allowing the implant to be easily cut and shaped as needed. The implant's shape mimics the contour of the cranium, with further tailoring available by soaking the implant in a hot, sterile saline bath for several minutes to relax the memory, and upon removal from the bath, bending it to assume a revised shape while it cools.



	A	B	C
OP9524	Cranial Grid	110mm x 97.5mm x 5.25mm	

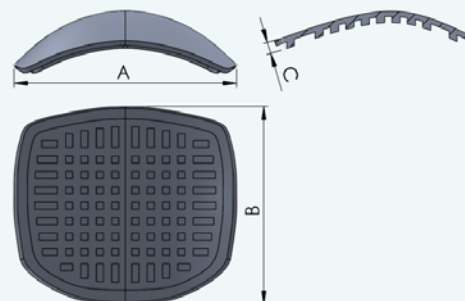


Cranial Hemisphere

The OMNIPORE Cranial Hemisphere is designed to be used for large cranial defects, providing surgeons with an off-the-shelf alternative to customized implants as well as complex grafts or other implant materials. The Cranial Hemisphere approximates the contour of a half cranium and can be trimmed with a blade to fit the defect. The edges can be delicately shaped and feathered using surgical scissors or a blade for a smooth transition between the implant and the patient's cranium. To fixate the implant, use sutures, surgical wire or craniofacial rigid fixation plates and screws.




	A	B	C
OP82000	Cranial Hemisphere – Right.....	174mm x 133mm x 5.0mm	
OP82001	Cranial Hemisphere – Left.....	174mm x 133mm x 5.0mm	

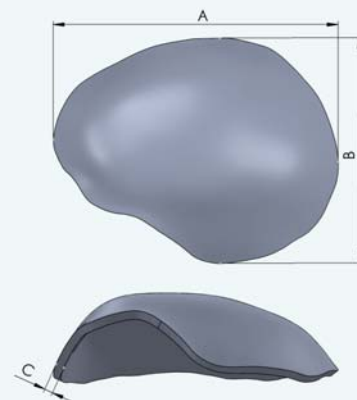

Blocks

OMNIPORE Blocks provide surgeons with ultimate flexibility in craniofacial augmentation and reconstruction. While in the sterile operating room, the surgeon can carve the blocks to meet individualized implant contours without worries of collapsing the pore structure. Soaking the implant in a hot, sterile saline bath for several minutes allows modification of the shape.

	A	B	C
OP6332	13mm x 38mm x 3.0mm	
OP6333	13mm x 38mm x 6.0mm	
OP6335	25mm x 50mm x 3.0mm	
OP6336	25mm x 50mm x 6.0mm	
OP6338	38mm x 63mm x 3.0mm	
OP6339	38mm x 63mm x 6.0mm	

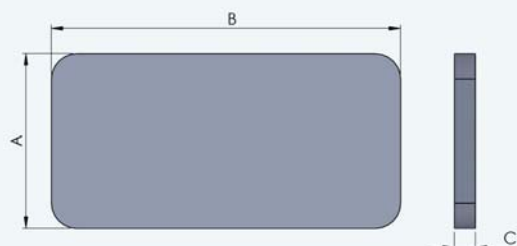

OMNIPORE® Customized Surgical Implants

Utilizing the latest and most innovative computer imaging and modeling technologies, Matrix Surgical USA can design precisely fitted patient-specific implants which:

- **Restore normal craniofacial anatomy**
- **Obliterate bony defects in the skull or orbits**
- **Augment facial skeletal or soft tissue defects**

Matrix Surgical USA specializes in the advanced modeling of **OMNIPORE** Customized Implants including the following case types:

COMPLEX ASYMMETRY

Asymmetry cases in which bilateral symmetry cannot be represented by a simple mid plane, where there is a significant amount of hardware already in place or when the bone surface has a very irregular surface.



SOFT TISSUE COMPENSATION

A hard implant is used to restore both a bony surface and missing soft tissue anatomy.



Key Features and Benefits

- Made from Porous High-Density Polyethylene, a biomaterial with a long history of use in craniofacial reconstruction and augmentation surgery.
- More precise fit compared to off-the-shelf options. Further refinements intra-operatively are possible with a scalpel or surgical scissors.
- Reduced surgery time.
- Can be stabilized with standard craniofacial fixation systems.
- Radiolucent. Minimal artifact on MRI scan.
- Patients do not experience sensitivity to extreme temperature changes as with titanium implants.
- Ability to accept CT Scan (DICOM) data via a secure, password-protected web portal.
- Provided sterile by Ethylene Oxide.
- Manufactured in the U.S.A.

OP89020	OMNIPORE Customized Cranial Implant
OP89021	OMNIPORE Customized Facial Implant
OP89022	Contralateral Charge for customized Facial Implant
OP89023	Skeletal Model of defect area
OP89024	Facial Implant Template non-sterile
OP89025	Cranial Implant Template non-sterile
OP89026	Contralateral Implant Template non-sterile


Complex defects, or defects involving the orbital structures or facial structures may require additional expense, time and/or a physical skull model and template.

CALL CUSTOMER CARE FOR FURTHER INFORMATION.


Orbital Volume Replacement and Enophthalmus Correction

Orbital Spheres

OMINPORE Spheres can be used for enucleation or evisceration procedures. OmniPore ocular implants are engineered to be macroporous to facilitate fibrovascular ingrowth, yet smoother on the exterior surface to reduce friction on the overlying soft tissue. Rectus muscles can be sutured directly to the surface of the implant obviating the need for a tissue wrap.

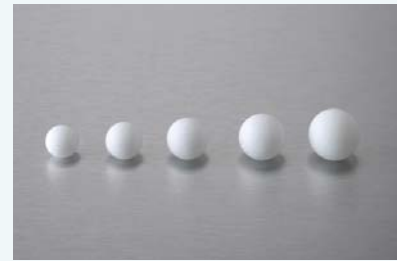


		Diameter
OP6316	Sphere	14mm
OP6326	Sphere	16mm
OP6327	Sphere	18mm
OP6317	Sphere	20mm
OP6322	Sphere	22mm



Ocular Conformers - Vented Only

Ocular Conformers are used after surgery to prevent closure or adhesions during the healing process. The small, convex-shaped acrylic devices have an internal surface that simulates the curvature of the orbit. Vented Conformers are available sterile in small, medium and large.


		A	B
OP9778	Vented - Small	22mm	19mm
OP9779	Vented - Medium	24mm	21mm
OP9780	Vented - Large	25mm	22mm



Enophthalmos Wedges

Enophthalmos Wedges help elevate and anteriorize the globe and provide volume to restore the orbit to its normal size and shape. Two sizes are available in left and right orientation.

		A	B	C
OP9541	Regular - Left	31mm	22mm	6.5mm
OP9542	Regular - Right	31mm	22mm	6.5mm
OP9543	Large - Left	39mm	28mm	7.5mm
OP9544	Large - Right	39mm	28mm	7.5mm

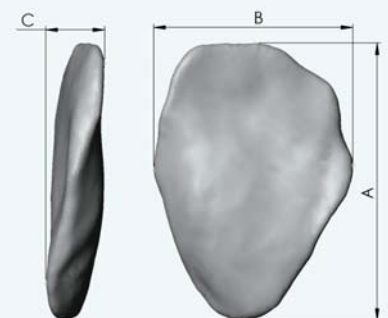

Orbital Floor Repair

OMNIPORE Sheets

OMNIPORE Sheets are used for craniofacial reconstruction and augmentation and are available in a variety of sizes and thicknesses. All Sheets come sterile and individually packaged and can be modified intraoperatively to conform to the skeleton. The 3S™ Sheets have a smooth superior surface which may prevent tissue attachment to the superior surface of the implant.



Micro Thin Sheet


	A	B	C
OP8438	30mm	50mm	0.45mm

Ultra Thin Sheets

OP7210	38mm	50mm	0.85mm
OP7212	50mm	76mm	0.85mm


Sheets

OP6330	38mm	50mm	1.5mm
OP6331	50mm	76mm	1.5mm
OP9562	38mm	50mm	3.0mm

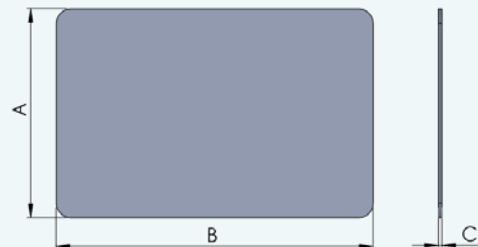

3S™ Sheets – Smooth Superior Surface


OP8312	38mm	50mm	1.0mm
OP9312	38mm	50mm	1.7mm

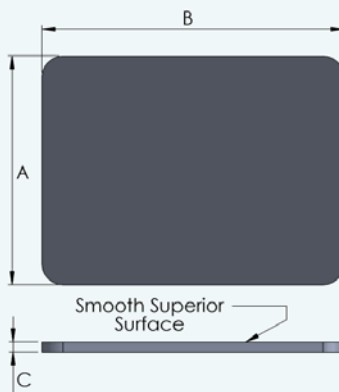

Channel Sheet

The OMNIPORE Channel Sheet is designed to repair significant orbital floor and wall trauma. The channels allow for placement with many sizes of rigid fixation plates and have been designed on angles so that the implant can be contoured and bent to the desired shape and still have fixation on strategic landmarks such as the inferior orbital rim, medial orbital wall and posterior ledge. The implant also comes with a smooth superior surface. *Channel Implant does not come with plates.*

	A	B	C
OP9530 Channel Sheet	50mm	50mm	2.0mm

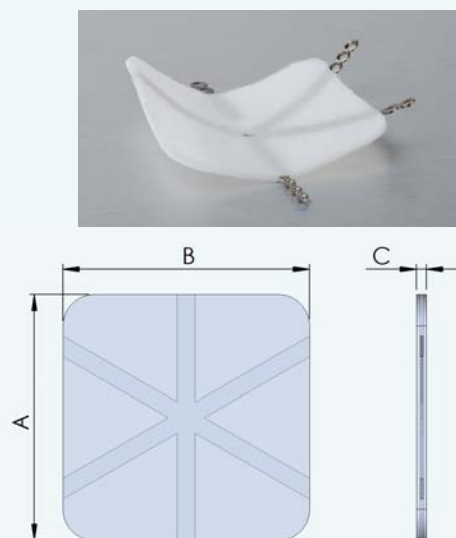

Terms and Conditions

To Order:

- All implants are shipped for two-day business delivery within the U.S. at no additional cost.
- Delivery times may vary according to freight delivery schedules.
- Delivery by any other service or carrier specified by the customer will be at the customer's expense.
- Current Price List pricing shall apply on invoiced product sales.
- Customized implants and surgical models are available upon request; order details, design requirements and lead times may be requested from Customer Care at 404-855-4592.

Return Goods Authorization (RGA):

- Prior authorization and a Return Goods Authorization (RGA) must be obtained from Matrix Surgical USA. Call Customer Care at 404-855-4592 to request an RGA.
- Freight charges for merchandise returned are the responsibility of the customer.
- Matrix Surgical USA allows the purchase of "back-up" implant products for surgery. Back-up implant products will be invoiced per the current price list. Requests for return and credit for back-up OMNIPORE™ Implant products less than \$2500 must be made within 60 days from date of invoice without penalty or restocking fee, provided the implants remain in the original unopened package.
- Returned product must be adequately packaged to prevent damage during the return shipment.
- A 20% restocking charge may apply to returns greater than \$2500 and must be returned within 60 days of date of invoice.

Credit and/or refund may *NOT* be issued for the following returns:

- Merchandise returned by other than original purchaser.
- Merchandise sold on a non-returnable basis, i.e. customized implants, shelf-pack quantities and non-implantable devices.
- Merchandise that has been opened, water damaged, crushed or otherwise damaged.
- Merchandise not returned in sellable condition.

No returns are allowed after 60 days from date of invoice.

Any merchandise returned other than in accordance with the above policies shall become the property of Matrix Surgical USA and will be dispositioned in an appropriate manner. The decision of Matrix Surgical USA with respect to the condition of the returned merchandise shall be final.

** All International Distributors should refer to their individual distribution agreement for specific terms and conditions.*

About Matrix Surgical USA

Matrix Surgical USA was founded in 2012 as a privately held company based in Atlanta, Georgia, USA. The company's core management team has deep domain expertise in the medical device industry and extensive experience with the design, development, production, marketing and global distribution of Porous High-Density Polyethylene Craniofacial Implants.

Matrix Surgical USA's flagship product is **OMNIPORE®** Surgical Implants, a biocompatible form of porous High-Density Polyethylene. The company offers more than 80 unique SKUs of various anatomical configurations and dimensions for reconstruction or augmentation of the craniomaxillofacial skeleton. Our products are available to healthcare providers in the United States and through a global network of stocking distributors in more than 35 countries around the world.

The founders created Matrix Surgical USA for one special reason: to be a specialty, niche-focused company that works in close collaboration with surgeons from all over the world to develop unique products that offer solutions to some of the most challenging clinical problems they face day in and day out. Our long history of success serving these client surgeons makes us a uniquely qualified partner and a fast growing company to watch.

Our Mission and Core Values

Matrix Surgical USA was created with the following core values in mind:

- To design, develop and introduce state-of-the-art products for reconstructive and aesthetic surgery that exceed customer expectations and recognized industry standards for quality and performance and the requirements of regulatory bodies from around the world.
- To recognize that our products play an important role in the healthcare practitioner's (HCP) ability to treat acquired (traumatic) or congenital diseases; hence, we are mindful of our responsibility to support HCPs in the proper selection and use of our products to help them achieve the best possible outcome for their patients.
- We know that everything we accomplish rests on the skills, integrity, commitment and dedication of our employees. We offer challenging and rewarding employment for our team members and set high expectations for performance.
- Matrix Surgical USA is committed to being a well-managed, results-oriented, innovation-driven organization whose team members have a passion for progress and a commitment to excellence. We constantly strive to be better partners with our customers and to be more connected, more forward-looking and more customer-focused than our competitors.
- We strive to be good corporate citizens by actively serving the best interests of the communities where we live and work as well as providing support to humanitarian organizations engaged in delivering vital health care services around the world.

MATRIX SURGICAL USA

Where Art Meets Science

OMNIPORE® Surgical Implants and Ocular Conformers are provided sterile by Matrix Surgical USA. DO NOT USE any implant or conformer if the package is open, damaged or wet. All STERILE items are considered single use and cannot be re-sterilized.

Surgeons should consult the package insert for instructions on the proper use and precautions for any OMNIPORE Surgical Implants or Ocular Conformers prior to use. For additional information worldwide, please contact your local OMNIPORE Surgical Implants Distributor; in the U.S., please contact Matrix Surgical USA directly using the information below.

Distributors should consult their distributor agreements for any claims.

All products manufactured and distributed by Matrix Surgical USA are latex free.

Matrix Surgical USA • 4025 Welcome All Road, Suite 120 • Atlanta, Georgia 30349 U.S.A.
T +1 404.855.4592 • F +1 404.344.0283 • info@matrixsurgicalusa.com • www.matrixsurgicalusa.com

CE Certificate Number US12/82636 ISO Certificate Number US12/82605